pH SOLUTIONS

CERTIFICATE OF ANALYSIS

261023-899-NHS-9

Issued Nov 4, 2026

SAMPLE

NAD 1000mg

Prepared for **GRX Bio-Science** · Lot **GBS-NAD1000-20261023-01**

PASS

ISO/IEC 17025:2017 ACCREDITED

A2LA R243 · PJLA Testing #84351 · Zero recalls since 2016

181 W Huntington Dr, Suite 181, Monrovia, CA 91016 · (818) 808-9757

BATCH / LOT	SAMPLE ID	MATRIX	PANELS RUN
GBS-NAD1000-20261023-01	261023-899-NHS-9	Peptide	3

RECEIVED	REPORTED	CLIENT
Oct 23, 2026	Nov 4, 2026	GRX Bio-Science

PEPTIDE PURITY

METHOD HPLC-UV @ 220 nm

ANALYTE	RESULT	UNIT	LIMIT	STATUS
NAD — purity	99.4	%		PASS

WATER ACTIVITY

METHOD Hygrometer (Rotronic HC2-AW)

ANALYTE	RESULT	UNIT	LIMIT	STATUS
Water activity	0.18	aw	< 0.65	PASS


MICROBIALS

METHOD qPCR

ANALYTE	RESULT	UNIT	LIMIT	STATUS
E. Coli	Not Detected		Not detected in 1 g	PASS
Salmonella spp.	Not Detected		Not detected in 1 g	PASS
Aspergillus flavus	Not Detected		Not detected in 1 g	PASS
Aspergillus fumigatus	Not Detected		Not detected in 1 g	PASS
Aspergillus niger	Not Detected		Not detected in 1 g	PASS
Aspergillus terreus	Not Detected		Not detected in 1 g	PASS

GRX distribution copy - client and lot labels updated by GRX; laboratory results unchanged.
Original client: Noble Harbor Sciences | Original lot: NHS-NAD1000-20261023-01

CHROMATOGRAM

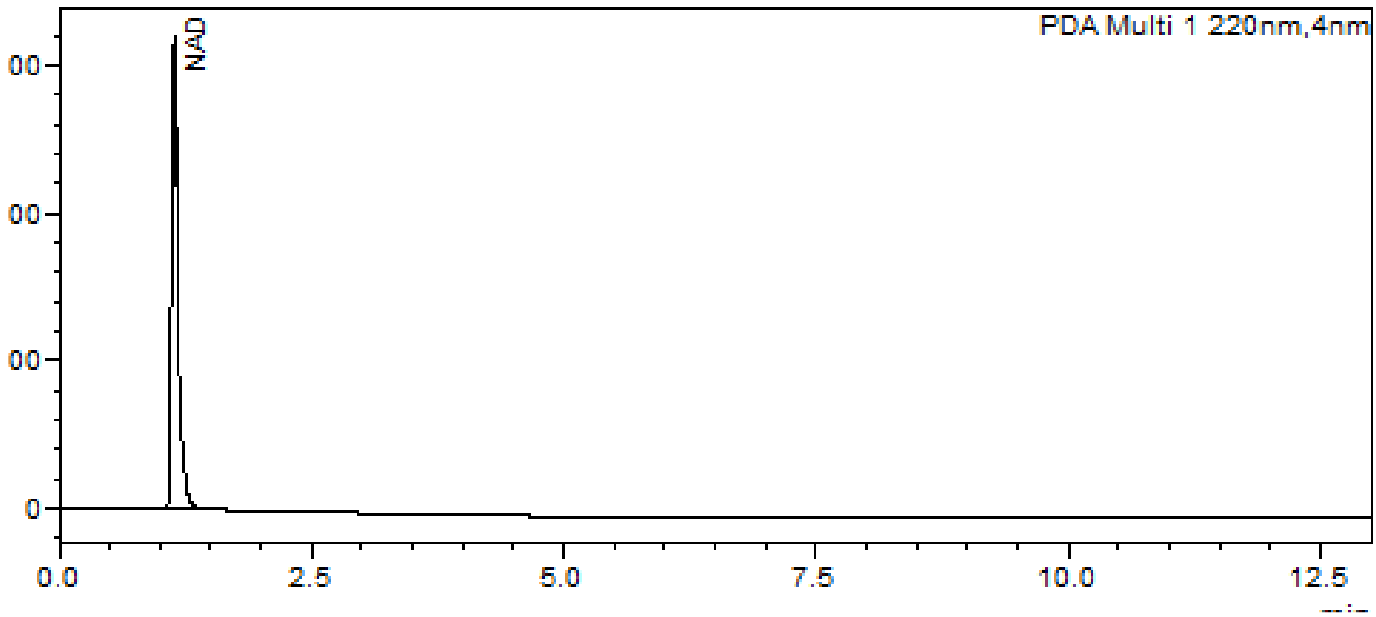

PH SOLUTIONS LAB INC.

Analysis performed in accordance with ISO/IEC 17025:2017. Results relate only to the sample as submitted. This certificate may not be reproduced except in full without the written approval of the laboratory. The online copy at the address beside is authoritative: if a printed COA disagrees with it, the online copy governs. Questions: info@phsolutionslab.com · (818) 808-9757.

SCAN TO VERIFY

www.phsolutionslab.com/coa/261023-899-NHS-9

GRX distribution copy - client and lot labels updated by GRX; laboratory results unchanged.
Original client: Noble Harbor Sciences | Original lot: NHS-NAD1000-20261023-01